


Eprouvette classe A | Measuring cylinder class A

- 1 | Graduation bleue
- 2 | Forme haute
- 3 | Avec bec
- 4 | Selon norme ISO 4788

- 1 | Blue graduation
- 2 | Tall form
- 3 | With spout
- 4 | According to ISO 4788 standard

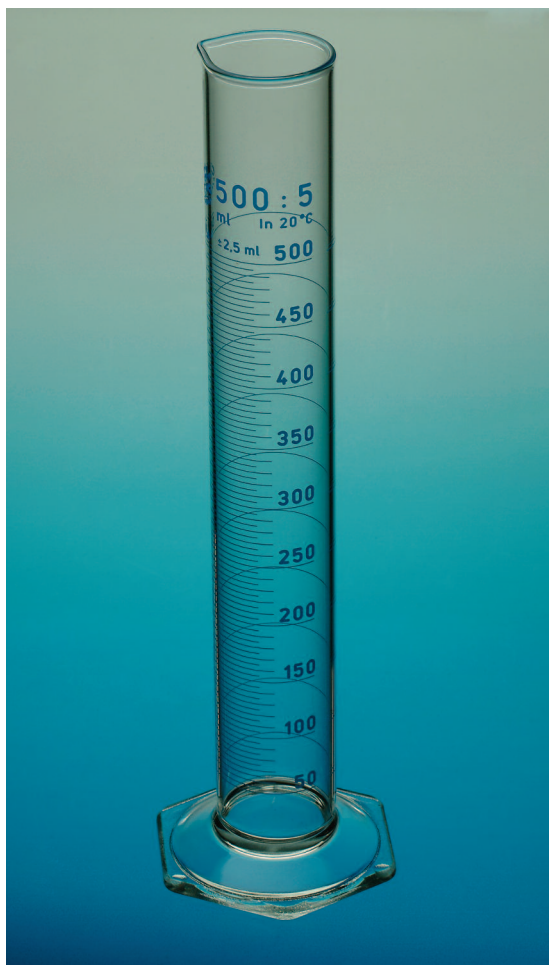

Référence	Volume	Graduation	Tolérance
Code	Volume	Graduation	Tolerance
00 285 005	5 mL	0,1 mL	± 0,10 mL
00 285 010	10 mL	0,2 mL	± 0,20 mL
00 285 025	25 mL	0,5 mL	± 0,50 mL
00 285 050	50 mL	1,0 mL	± 1,00 mL
00 285 100	100 mL	1,0 mL	± 1,00 mL
00 285 250	250 mL	2,0 mL	± 2,00 mL
00 285 500	500 mL	5,0 mL	± 5,00 mL
00 285 600	1000 mL	10,0 mL	± 10,0 mL
00 285 700	2000 mL	20,0 mL	± 20,0 mL